
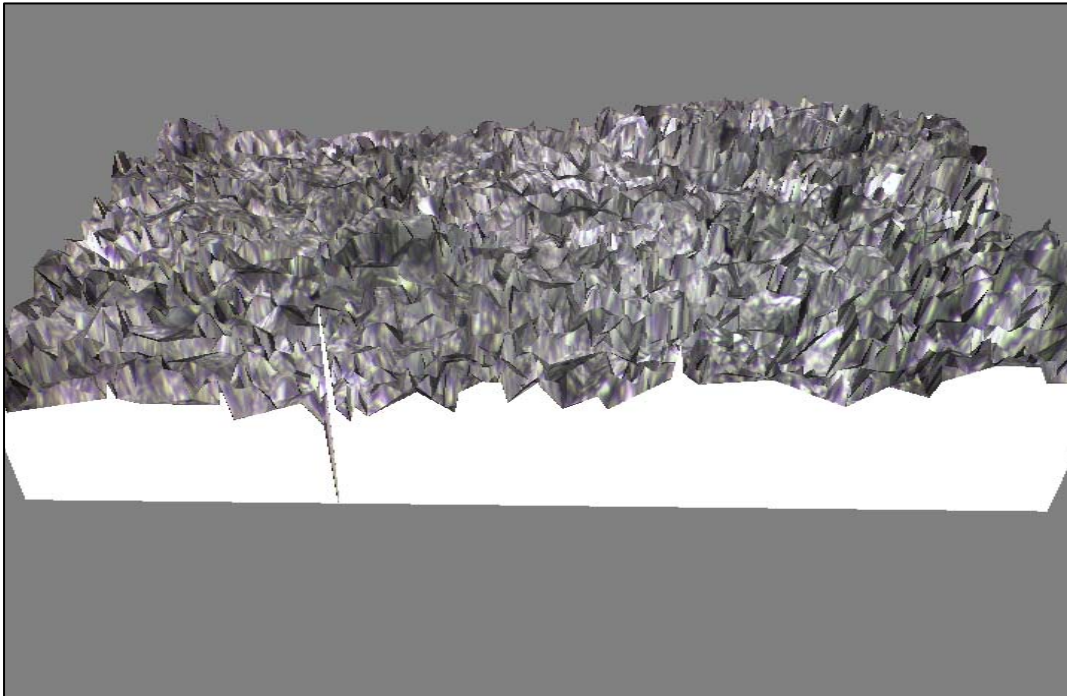


Area Roughness Evaluation as per ASME B46.1

Date:		Units: microns
Laboratory:	Clemex Technologies	Magnification: 50x
Department:	Quality Control	Calibration: 2.6000 $\mu\text{m}/\text{pixel}$
User:		# of fields: 1
Sample ID:	Area on 3D	Field Area: 9692650.24

	Rq	Ra	Rt	Rp	Rv	Lx	Ly	Area	N
Roughness	16.47	13.48	116.26	52.59	-63.67	3551.60	2633.80	9354205	7600

Distance from the mean plane in default units

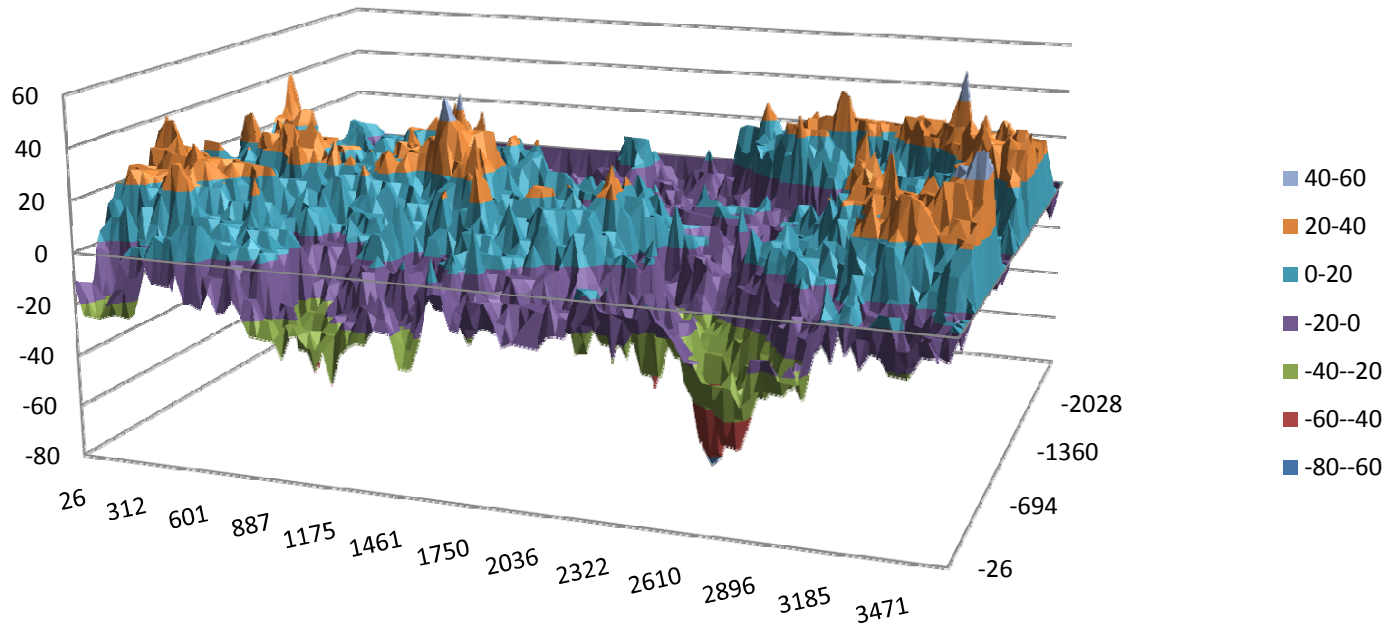

Comments: