
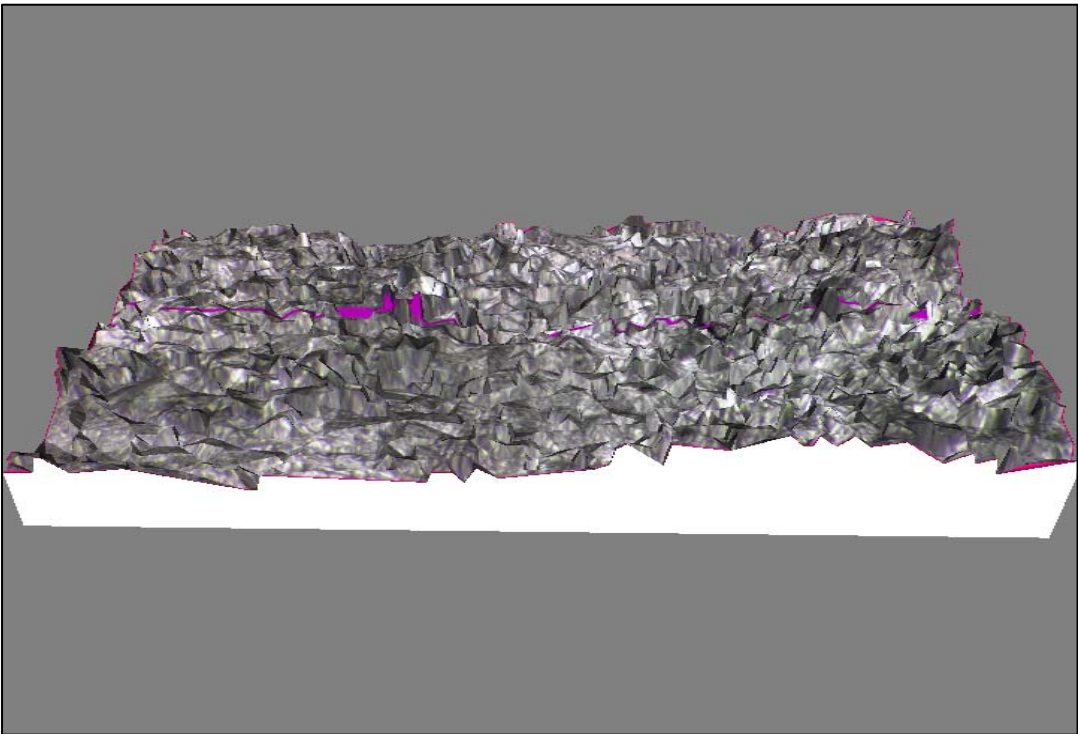


Linear Roughness Evaluation as per ASME B46.1

Date:		Units: microns
Laboratory:	Clemex Technologies	Magnification: 2500
Department:	Quality Control	Calibration: 2.6000 $\mu\text{m}/\text{pixel}$
User:		# of fields: 1
Sample ID:	Linear on 3D	Field Area: 9692650.24

	Rq	Ra	Rt	Rp	Rv	L	N
Roughness	14.78	11.62	70.54	33.46	-37.08	3528.20	240

Distance from the mean in default units

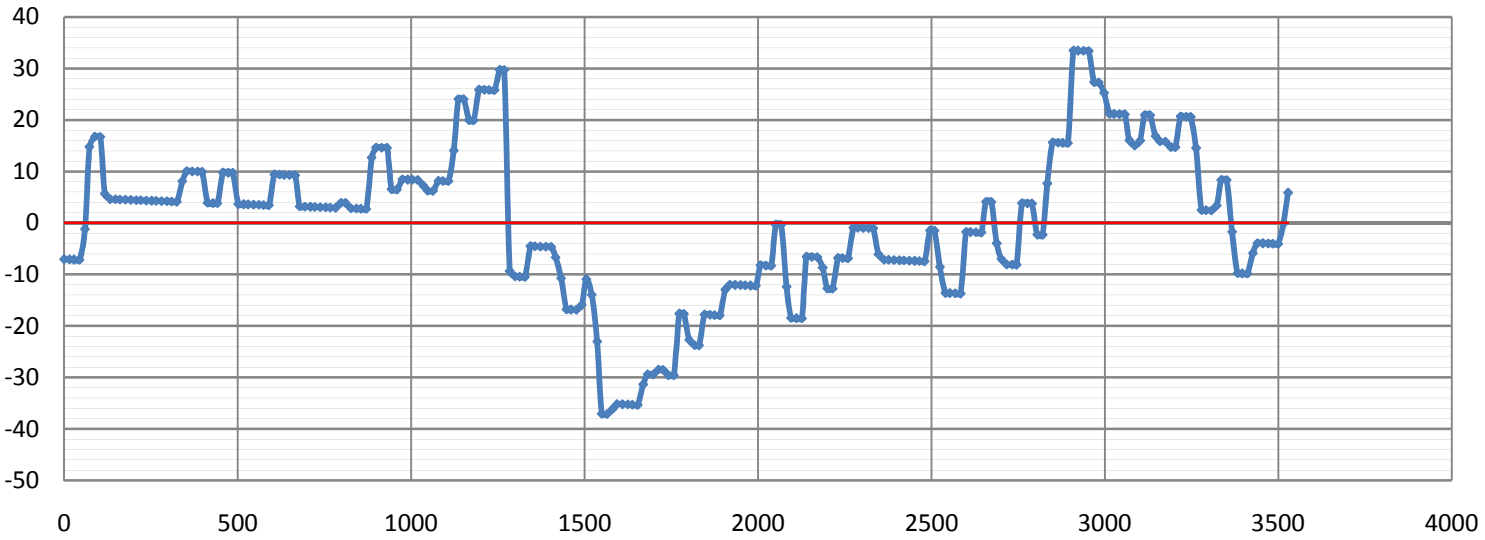

Comments: