

Date: 2026-juil.-15, 09:47:04 GMT-04:00
Company: Clemex
User: Clemex Support (2026-Jun-30 10:21:48 GMT-04:00)

Calibration: 0,2302 $\mu\text{m}/\text{pixel}$
Units: Microns
Field count: 1
Points of test grid: 16
Field area (μm^2): 16281,39
Tot. area (μm^2): 16281,39

Sample ID:
Magnification: 400x

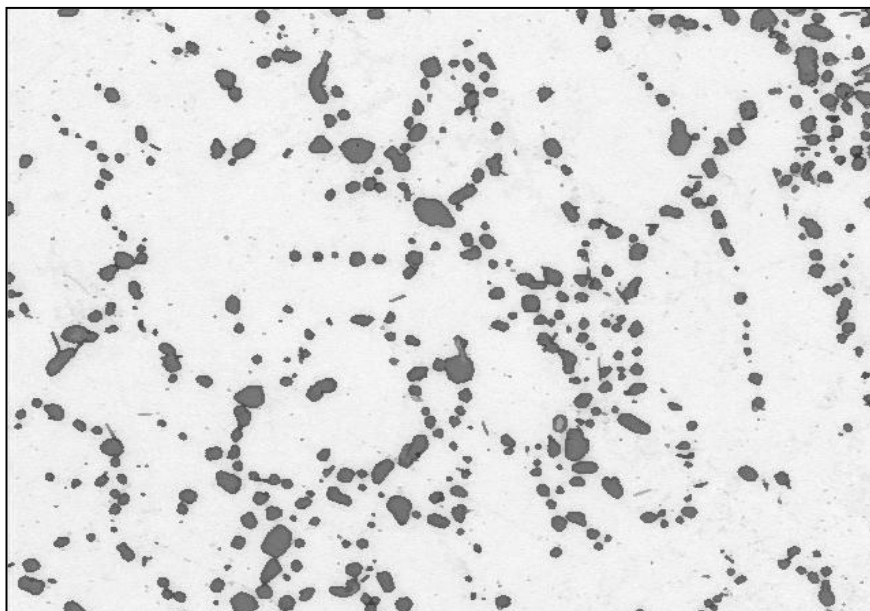


Figure 1: Last field of view analyzed.

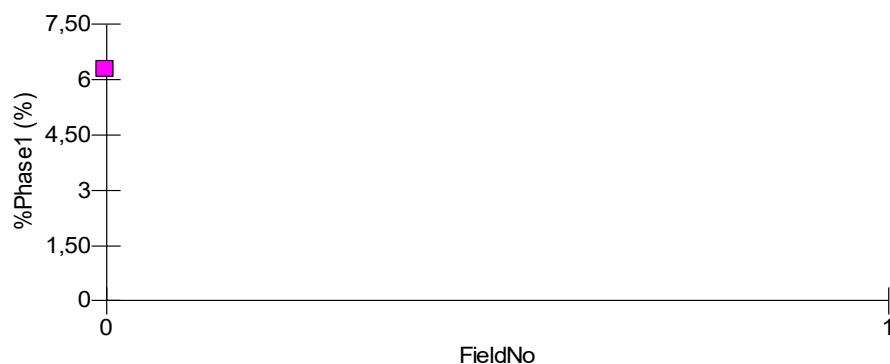


Chart 1: Volume fraction estimated of phase 1

Results

Volume fraction V_V (%): 6,25